



WEB[®]
Aneurysm Embolization System

PRODUCT SPECIFICATION & ORDERING GUIDE



SL Device





SLS Device

Aneurysm Therapy Solutions

Device Selection Tables


WEB® SL Device Selection Table

Treat Aneurysms Between 3mm and 10mm

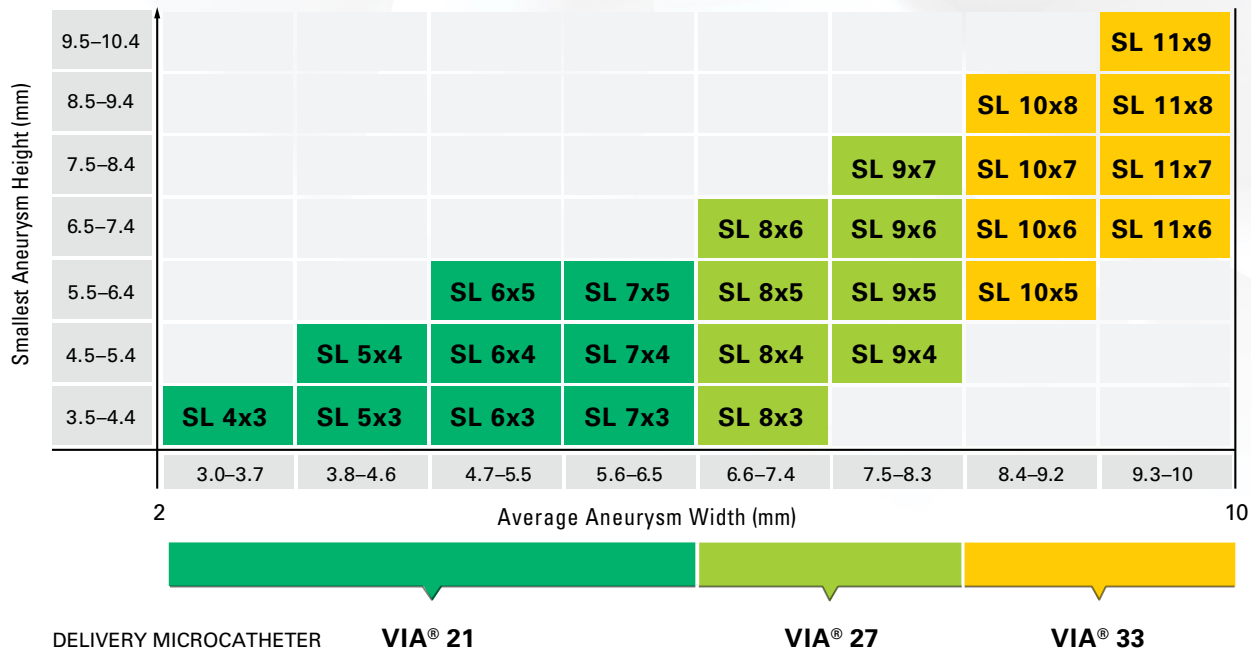


WEB® SLS Device Selection Table

Treat Aneurysms Between 3mm and 10mm

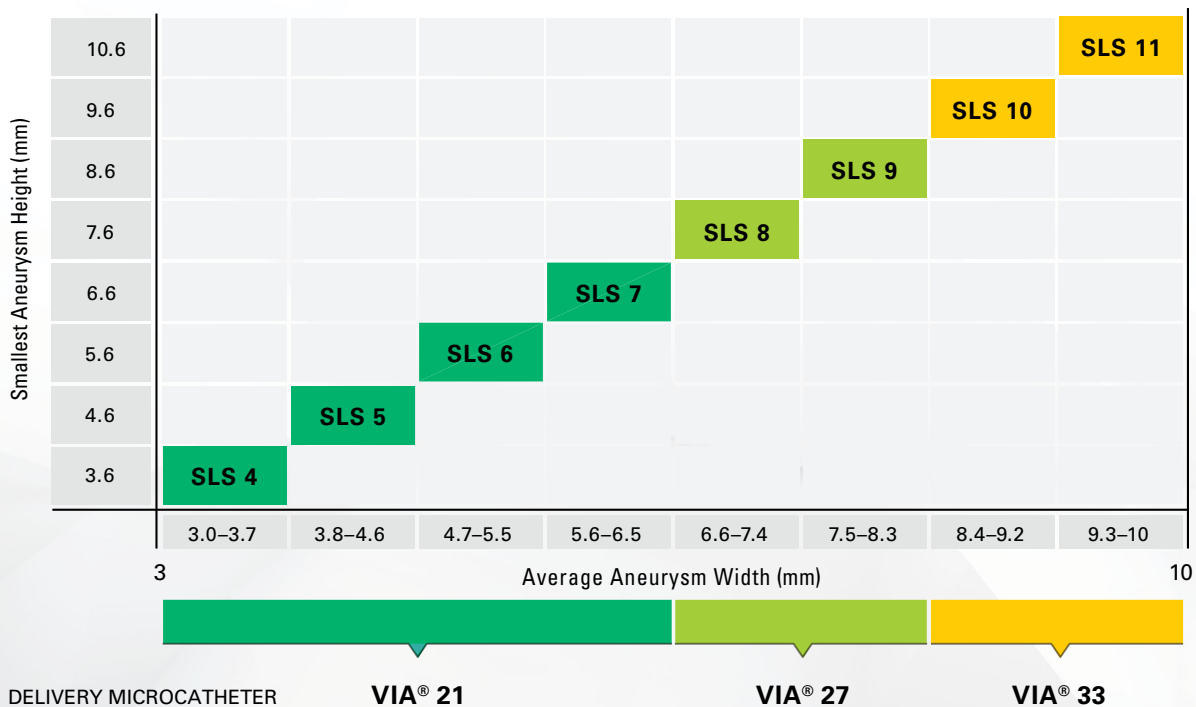


WEB® System Part Numbers

WEB® SL



	Name	Ref No.	Diameter (mm)	Height (mm)
VIA® 21	WEB SL 4 x 3	W4-4-3	4	3
	WEB SL 5 x 3	W4-5-3	5	3
	WEB SL 5 x 4	W4-5-4	5	4
	WEB SL 6 x 3	W4-6-3	6	3
	WEB SL 6 x 4	W4-6-4	6	4
	WEB SL 6 x 5	W4-6-5	6	5
	WEB SL 7 x 3	W4-7-3	7	3
	WEB SL 7 x 4	W4-7-4	7	4
VIA® 27	WEB SL 7 x 5	W4-7-5	7	5
	WEB SL 8 x 3	W2-8-3	8	3
	WEB SL 8 x 4	W2-8-4	8	4
	WEB SL 8 x 5	W2-8-5	8	5
	WEB SL 8 x 6	W2-8-6	8	6
	WEB SL 9 x 4	W2-9-4	9	4
	WEB SL 9 x 5	W2-9-5	9	5
	WEB SL 9 x 6	W2-9-6	9	6
VIA® 33	WEB SL 9 x 7	W2-9-7	9	7
	WEB SL 10 x 5	W2-10-5	10	5
	WEB SL 10 x 6	W2-10-6	10	6
	WEB SL 10 x 7	W2-10-7	10	7
	WEB SL 10 x 8	W2-10-8	10	8
	WEB SL 11 x 6	W2-11-6	11	6
	WEB SL 11 x 7	W2-11-7	11	7
	WEB SL 11 x 8	W2-11-8	11	8


WEB® SLS



VIA® 21	WEB SLS 4	W4-4-S	4	2.6
	WEB SLS 5	W4-5-S	5	3.6
	WEB SLS 6	W4-6-S	6	4.6
	WEB SLS 7	W4-7-S	7	5.6
VIA® 27	WEB SLS 8	W2-8-S	8	6.6
	WEB SLS 9	W2-9-S	9	7.6
VIA® 33	WEB SLS 10	W2-10-S	10	8.6
	WEB SLS 11	W2-11-S	11	9.6

VIA® Microcatheter

Name	Ref No.	(A) ID (inch)	(B) Distal OD (French)	(C) Proximal OD (French)	(D) Working Length (cm)	Tip Markers
VIA® 21	VIA-21-154-01	0.021"	2.5F	2.8F	154 cm	1
VIA® 27	VIA-27-154-01	0.027"	3.0F	3.2F	154 cm	1
VIA® 33	VIA-33-133-01	0.033"	3.4F	3.8F	133 cm	1

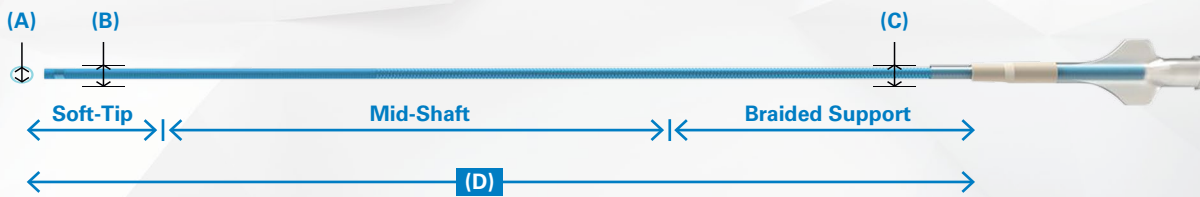

WEB® Detachment Controller


Name	Ref No.
WDC: WEB® Detachment Controller (5 per box)	WDC-1



WEB[®]

Aneurysm Embolization System

Stable Distal Access:
Triaxial technique

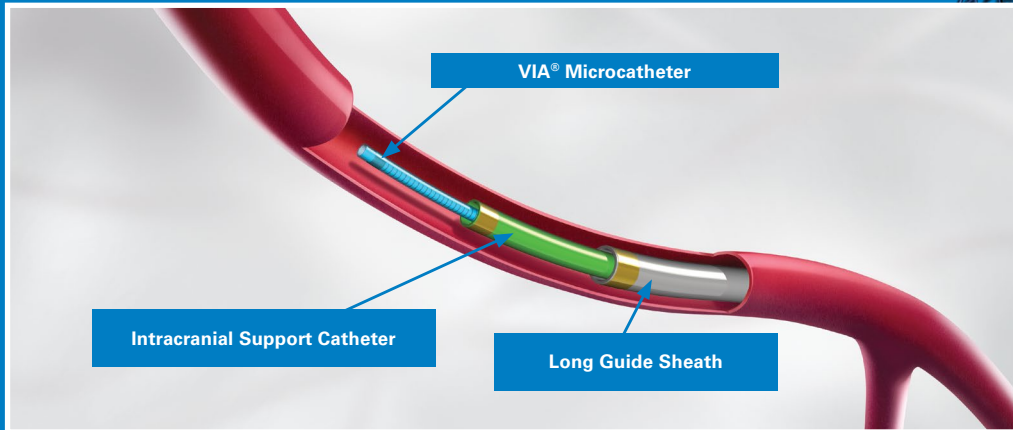

Device Compatibility

WEB [®] SL/SLS Device Width (mm)	VIA [®] Microcatheter (Delivery Catheter)	Intracranial Support Catheter	Long Guide Sheath
4-7	VIA[®] 21 ID: 0.021" / 1.6F / 0.53 mm Distal OD: 2.5F / 0.033" / 0.84 mm Proximal OD: 2.8F / 0.036" / 0.91 mm Length: 154 cm	5F, 0.056" ID or larger, 90 – 125 cm long	6F: 80 / 90 cm long
8-9	VIA[®] 27 ID: 0.027" / 2.1F / 0.69 mm Distal OD: 3.0F / 0.039" / 0.99 mm Proximal OD: 3.2 F / 0.042" / 1.07 mm Length: 154 cm	6F, 0.070" ID or larger, 90 – 125 cm long	6F: 80 / 90 cm long
10-11	VIA[®] 33 ID: 0.033" / 2.5F / 0.84 mm Distal OD: 3.4F / 0.045" / 1.14 mm Proximal OD: 3.8F / 0.050" / 1.27 mm Length: 133 cm	6F, 0.070" ID or larger, 90 – 115 cm long	6F: 80 / 90 cm long

INDICATIONS FOR USE:

The WEB Aneurysm Embolization System is indicated for use at the middle cerebral artery (MCA) bifurcation, internal carotid artery (ICA) terminus, anterior communicating artery (AComm) complex, or basilar artery apex for the endovascular treatment of adult patients with saccular, wide neck bifurcation intracranial aneurysms with dome diameter from 3 mm to 10 mm and either neck size 4 mm or greater or the dome-to-neck ratio is greater than 1 and less than 2.

The WEB Aneurysm Embolization System is contraindicated for patients with known bacterial infection that may interfere with or negatively affect the implantation procedure and patients with known hypersensitivity to nickel. For complete indications, contraindications, potential complications, warnings, precautions, and instructions, see instructions for use (IFU provided with the device).

The VIA[®] Catheter is intended for the introduction of non-liquid interventional devices (such as stents/flow diverters) and infusion of diagnostic (such as contrast media) or non-liquid therapeutic agents into the neuro, peripheral, and coronary vasculature. The VIA Catheter is contraindicated for use with liquid embolic materials, such as n-butyl 2-cyanoacrylate or ethylene vinyl alcohol & DMSO (dimethyl sulfoxide). The VIA Catheter is contraindicated for use in the pediatric population (<22 yrs of age).

Caution: Federal law restricts these devices to sale by or on the order of a physician

MICROVENTION[®] is a registered trademark of MicroVention, Inc. WEB[®] and VIA[®] are registered trademarks of Sequent Medical, Inc. ©2019 MicroVention, Inc. MM768 US 1/19



**MicroVention Worldwide
Innovat[®] Center** 1.714.247.8000
35 Enterprise
Aliso Viejo, CA 92656 USA
Customer Service 1.800.990.8368
Web microvention.com